

Series: 3576

Report Name: original

Chromaster System Manager Report

Analyzed Date and Time: 25/03/2022 13:41

Processing Method: Test KV

Sample Name: CBD 10% cucuma


Injection from this vial: 1 of 1

Series: 3576

Vial Number: 1

Vial Type: UNK

Volume: 10,0 ul

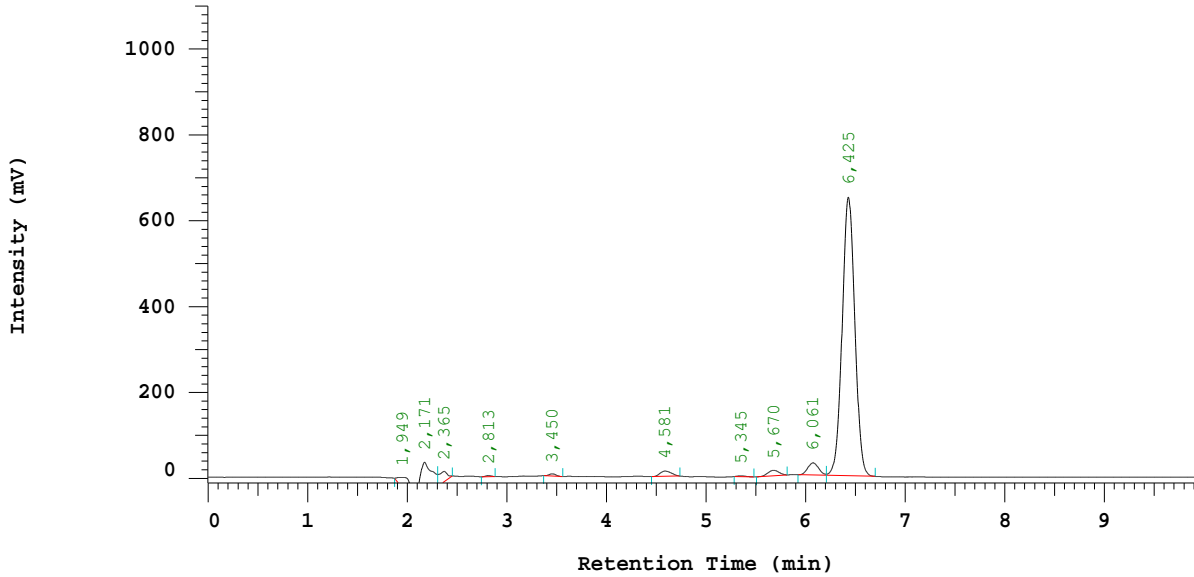

RT	Area	Conc 1	Name
1,949	254267	0,000000	
2,171	653879	0,000000	
2,365	152349	0,000000	
2,813	9621	0,000000	
3,450	25543	0,000000	
4,581	97844	0,000000	
5,345	10980	0,000000	
5,670	97543	0,000000	
6,061	213909	0,745000	CBDA
6,425	5735670	10,094000	CBD
	7251605	10,839000	

Peak rejection level: 0