

Series: 3578

Report Name: original

### Chromaster System Manager Report

Analyzed Date and Time: 25/03/2022 14:33

Processing Method: Test KV

Sample Name: CBD 10% melissa


Injection from this vial: 1 of 1

Series: 3578

Vial Number: 1

Vial Type: UNK

Volume: 10,0 ul

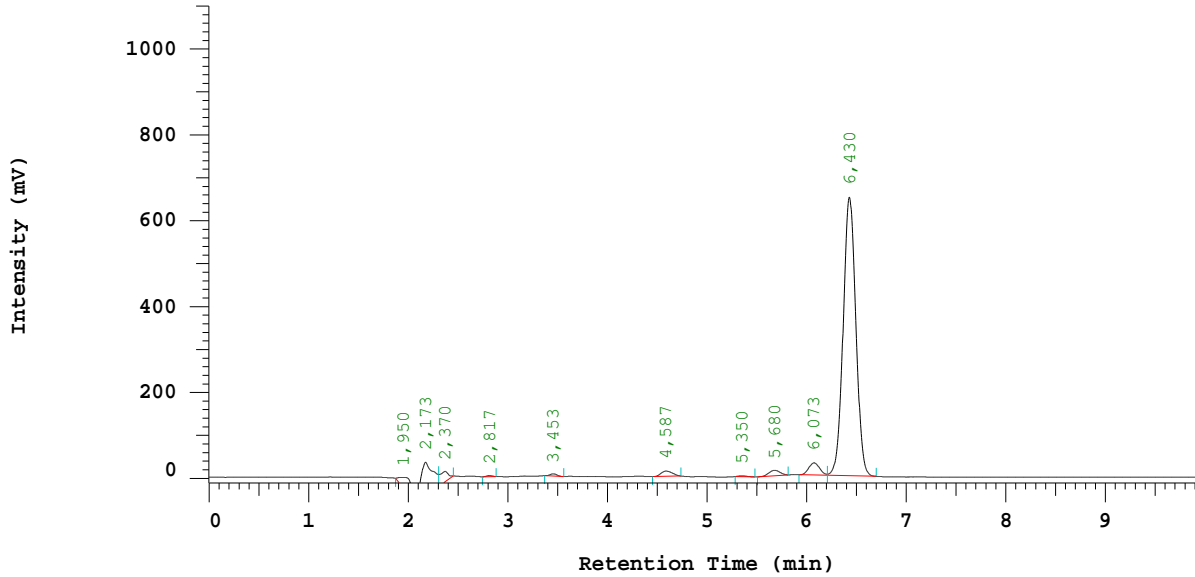

RT	Area	Conc 1	Name
1,950	255366	0,000000	
2,173	654514	0,000000	
2,370	153444	0,000000	
2,817	9792	0,000000	
3,453	25937	0,000000	
4,587	98011	0,000000	
5,350	10936	0,000000	
5,680	97703	0,000000	
6,073	215756	0,751000	CBDA
6,430	5746568	10,113000	CBD
	7268027	10,864000	

Peak rejection level: 0